

# Forearm Skin Tissue Dielectric Constant: Effect of Changes in Vascular Volume and Skin Blood Perfusion

Xiaoran Guo<sup>1</sup>, OMS-3; Mark Salmon<sup>1</sup>, OMS-3; Matt Uhde<sup>1</sup>, OMS-3; Harvey N. Mayrovitz<sup>2</sup>, PhD

<sup>1</sup>College of Osteopathic Medicine, Nova Southeastern University, Fort Lauderdale, FL

<sup>2</sup>College of Medical Sciences, Department of Physiology, Nova Southeastern University, Fort Lauderdale, FL

## Background

Measurements of local tissue dielectric constant (TDC) via the open-ended coaxial probe method are useful non-invasive measures of local tissue water<sup>[1-6]</sup>. The method permits assessment and tracking of changes in skin tissue water in many situations including lymphedema<sup>[7]</sup> and other conditions<sup>[8-12]</sup>. The operating principle depends on the direct relationship between TDC values and fluid content within measured tissue to effective depths up to about 5 mm below the epidermal surface. This depth includes dermal tissues as well as vascular structures so there is a question as to affects of blood volume and skin blood flow (SBF) on TDC values obtained. Our objective is to determine the extent to which local blood volume and SBF effect measured TDC values.

## Methods

TDC values to a depth of about 1.5 mm and SBF to a similar depth via laser-Doppler flowmetry were measured on the anterior forearms of 20 young adult healthy supine subjects (10 male) under two test conditions. Test 1 was done with the arm horizontal and then passively raised to about 90° for 5 minutes. Test 2 was done with the arm horizontal before and during a 5 minute upper arm cuff compression to a pressure of 50 mmHg. SBF was also measured on the 3rd finger pad during all maneuvers. The forearm target site was 8 cm distal to the antecubital fossa.



Pictured below: SBF measurements taken passively with the arm at rest and BP cuff inflated to 50 mmHg.



Pictured above: A TDC measurement taken by the experimenter with the arm at rest and BP cuff inflated to 50 mmHg.

## Results

Forearm Tissue Dielectric Constants




Figure 1 p<.0001

Forearm Skin Blood Flow




Figure 2 p=.008

Test 1 Test 2

Figure 2. Skin blood flow (SBF) at the forearm site measured by laser-Doppler flowmetry. SBF was significantly increased with arm raising (Test 1) and significantly decreased with application of 50 mmHg pressure proximal to the bicep (Test 2).

Finger Skin Blood Flow




Figure 3 p<.0001

Figure 3 p=.016

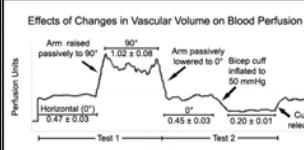


Figure 4. Tracking forearm SBF values as Test 1 and Test 2 maneuvers are performed sequentially for one subject. SBF values are elevated with arm raising (Test 1); following a return to baseline when the arm is lowered, SBF values are decreased with application of 50 mmHg of pressure to the bicep (Test 2).

## Conclusions

Over the wide range of blood volume and SBF shifts associated with the employed maneuvers a 3.0-3.5% change in TDC values was observed. This suggests that for most clinical evaluation and tracking purposes in which such large shifts in blood volume and perfusion are unlikely, the confounding effects of variations in SBF or volume are inconsequential. From the physiological perspective, the decrease in TDC with arm raising is consistent with a gravity-dependent drainage in vascular volume and the increase in TDC with application of cuff pressure is consistent with reduced drainage from vascular compression.

The finding of an increase in forearm SBF agrees with previous work suggesting that venous emptying leads to arteriolar vasodilation. The decrease in SBF at forearm with cuff pressure and at finger with arm raise is consistent with a perfusion pressure reduction accompanying these maneuvers.

## References

- Lahtinen T, Nuutilainen J, Alelanen E, Turunen M, Nuortio L, Usenius T, et al. Quantitative assessment of protein content in irradiated human skin. International journal of radiation oncology, biology, physics. 1999; 43: 635-8.
- Alanen E, Lahtinen T, Nuutilainen J. Measurement of dielectric properties of subcutaneous fat with open-ended coaxial sensors. Phys Med Biol 1998; 43: 475-485.
- Alanen E, Lahtinen T, Nuutilainen J. Variational formulation of open-ended coaxial line in contact with layered biological medium. IEEE Trans Biomed Eng 1998; 45: 1241-1248.
- Nuutilainen J, Ikaheimo R, Lahtinen T. Validation of a new dielectric device to assess changes of tissue water in skin and subcutaneous fat. Physiological Measurement. 2004; 25: 447-54.
- Stuchly MA, Athey TW, Samaras GM, Taylor G. Measurement of radio frequency permittivity of biological tissues with an open-ended coaxial line: Part II - Experimental Results. IEEE Trans Microwave Theory Tech 1982; 30: 87-92.
- Amoto A, Matsumoto T. Noninvasive method for measuring the electrical properties of deep tissues using an open-ended coaxial probe. Medical engineering & physics. 1996;18: 641-646.
- Stuchly Ma, Athey TW, Stuchly SS, Samaras GM, Taylor G. Dielectric properties of animal tissues in vivo at frequencies 10 MHz-1 GHz. Bioelectromagnetics. 1981; 2: 93-103.
- Mayrovitz HN, Weingrad DN, Davey S. Local tissue water in at-risk and contralateral forearms of women with and without breast cancer treatment-related lymphedema. Lymphatic research and biology. 2009; 7: 153-8.
- Laakkonen DE, Nuutilainen J, Lahtinen T, Rissanen a, Niskanen LK. Changes in abdominal subcutaneous fat water content with rapid weight loss and long-term weight maintenance in abdominally obese men and women. International journal of obesity and related metabolic disorders : journal of the International Association for the Study of Obesity. 2003; 27: 677-83.
- Petäjä L, Nuutilainen J, Uusaro A, Lahtinen T, Ruokonen E. Dielectric constant of skin and subcutaneous fat to assess fluid changes after cardiac surgery. Physiological measurement. 2003; 24: 383.
- Mayrovitz HN, Carson S, Luis M. Male-female differences in forearm skin tissue dielectric constant. Clinical physiology and functional imaging. 2010; 30: 328-32.
- Mayrovitz HN, Luis M. Spatial variations in forearm skin tissue dielectric constant. Skin research and technology 2010; 16: 438-43.
- Mayrovitz HN. Local tissue water assessed by measuring forearm skin dielectric constant: dependence on measurement depth, age and body mass index. Skin research and technology 2010; 16: 16-22.